



Strategic Diagnostics Inc.



Test and Be Sure

Trait ✓ Cry34Ab1 Test Kit

Part Number 7000055

Bulk Grain Testing



Intended Use

The intended use of the kit is the qualitative (yes/no) determination of the Cry34Ab1 protein in corn grain samples. The Trait ✓ Cry34Ab1 test strip has been performance certified by USDA GIPSA for detection limit of one (1) HERCULEX™ RW or HERCULEX™ XTRA corn kernel in 800 non-HERCULEX kernels. This kit has been validated and approved by Dow AgroSciences for the detection of the HERCULEX trait.

Product Description

The Trait ✓ Cry34Ab1 Lateral Flow Test Kits detect the Cry34Ab1 protein produced by a gene derived from *Bacillus thuringiensis* (*Bt*). This gene has been incorporated into insect-resistant corn including HERCULEX™ RW and HERCULEX™ XTRA. The lateral flow strips and other kit components are sufficient to detect the presence or absence of the Cry34Ab1 protein in both field and laboratory environments. Different application protocols are required for leaf, seed and bulk grain detection. This product can screen HERCULEX™ RW (DAS59122-7) corn grain at specified levels.

Principle of the Test

The assay uses a double antibody sandwich format. Antibodies specific to the Cry34Ab1 protein are coupled to a color reagent and incorporated into the lateral flow strip. When the lateral flow strip is placed in a small amount of an extract from plant tissue that contains Cry34Ab1 protein, binding occurs between the coupled antibody and the protein. A sandwich is formed with some, but not all the antibody that is coupled to the color reagent. The membrane contains two capture zones, one captures the bound Cry34Ab1 protein and the other captures color reagent. These capture zones display a reddish color when the sandwich and/or unreacted colored reagents are captured in the specific zones on the membrane. The presence of only one line (control line) on the membrane indicates a negative sample and the presence of two lines indicates a positive sample.

Contents of Kit

Description	Quantity
Trait ✓ Cry34Ab1 Lateral Flow Test Strips	2x50*
Sample Tubes (1.5 ml)	100*
Transfer pipettes	100*
User Guide	1

* May contain more than 100 units.

Materials Required but not Supplied

Laboratory grade blender (Waring Model 31BL91 recommended; SDI P/N 6000022)
 Waring adapter for "Mason-type" glass jars (6000021)
 Blender jars ("Mason-type"; 4, 8, 16 and 32 oz.)
 Sample tube rack (6000023)
 Graduated cylinder, 250 ml (6000024)
 Blender Shield (P/N 6000037)
 Methanol (laboratory grade)

Preparation and Storage of Reagents

The Trait ✓ Cry34Ab1 Corn Grain Test Kit should be stored at room temperature. The Trait ✓ Cry34Ab1 Test Strips used in this kit must be kept in the canister with the desiccant. The moisture indicator card must be blue in color. If the moisture indicator card is pink, please contact SDI Technical Services. Storage conditions higher than room temperature may adversely affect performance.

Sampling

The samples used for the Trait ✓ Cry34Ab1 Corn Grain Test Kit can be sub-samples of those "representative samples" collected from trucks, railcars, barges, etc. for other tests. The size of the sub-samples to be used for the Trait ✓ Cry34Ab1 test will depend on the percent Cry34Ab1 screening level desired and an acceptable level of risk that the Cry34Ab1 level is close to the screening level. The number and size of the sub-samples will be discussed in more detail in the **Principle of the Screening Application** section.

Note: It is assumed that the samples collected are representative of the contents of the truck or container and are sufficiently mixed to contain a random distribution of the sample contents.

Sample Preparation: Weighing the Sample

The statistical sampling plan (see **Principle of the Screening Application**) is dependent on the number of corn kernels used. However, it is more practical for routine testing to weigh corn kernels instead of counting to obtain the desired number of kernels. The average weight of corn kernels depends on the variety of corn and environmental conditions.

It is recommended that the weight-to-corn kernel ratio for each variety be determined as follows.

1. Count 100 kernels of the variety to be tested.
2. Weigh the 100 kernels to the nearest 0.01 gram.
3. Divide the weight of the corn kernels by 100 to get the average grams per kernel.
4. Multiply this average weight by the desired number of corn kernels in the sub-samples (selected in **Tables C, D or E**) to determine the weight for the sub-samples.
5. Construct a weight-to-corn kernel ratio table for each variety for the different sub-sample sizes to be used.

Example: One hundred (100) corn kernels of Variety X weigh 25.00 grams. Each corn kernel then weighs 0.25 grams. Multiply the 0.25-gram per corn kernel times the number of corn kernels in each sample size to get the following table.

Table A: Example: Weight-to-Kernel Ratio

No. Corn Kernels (a)	Grams per Sample of X			
	100	400	600	800
Sample Weight (g)	25	100	150	200

(a) From Tables C, D and E.

This average weight is then used to obtain the number of corn kernels for this corn variety.

Sample Preparation

The corn sample is ground and then extracted with water in a glass “Mason”-type jar. The sample preparation is important for the proper function of the test, especially the ratio of water to the weight of the corn sample. The volume of water in milliliters (mL) should be close to 1.25 times the weight of corn sample in grams (g). The size of “Mason” jar required and the grinding time depends on the sample size to be analyzed. **Table B** lists those parameters.

Table B: Parameters for Preparing Samples

Number of Kernels in Sample	Jar Size (oz.)	Grind Time (sec)
25-125	4	10-20
125-250	8	15-25
250-500	16	20-35
>500	32	45-60

The processing parameters were determined using the laboratory grade Waring Model 31BL91 food processor with the standard blade (see **Materials Required but not Supplied**). Other food processors may require different parameters.

Sample Processing

1. Weigh sub-samples from each truck or container.
2. Place each sub-sample in a clean, **dry** “Mason” jar of the appropriate size. See **Table B**.
3. Attach the jar adapter and clean, **dry** cutting blades.
4. Place the jar onto the food processor, place a shield over the jar and grind the sub-sample on high speed for the time indicated in **Table B**.

Caution: It is recommended to shield the jars during grinding with a “tri-cornered” 1-liter plastic beaker (P/N 6000037).

5. Remove the adapter and cutting blades.
6. Add the volume of water (see below) to the ground corn in the jar, place a lid on the jar and shake the jar until all the ground corn is well wetted (about 10-20 sec.).

Sample Weight (g) X 1.25 = Water Volume (mL)


Note: The sample will have a “thick” consistency but should contain some free liquid after a short settling time. **There should be no whole kernels remaining.**

7. Use this free liquid as sample in the **Test Procedure**.



Test Procedure


1. Transfer the liquid from the sample prepared to a sample tube by squeezing the bulb of the transfer pipette and inserting it in the free liquid in the top of the sample jar.
2. Release the bulb to pull up the sample. Add the sample from the pipette to the sample tube by squeezing the bulb. This should be approximately 0.5 mL.



The sample tube has a 0.5-mL indicator at the top of the tapered section.

3. Place one Trait[✓] Cry34Ab1 Test Strip into the sample tube. Let sit for 5 minutes.
4. The appearance of **one line** (control) on the strip indicates a **negative** result.
5. The appearance of **two lines** on the strip indicates a **positive** result.

Illustration of Test Strip

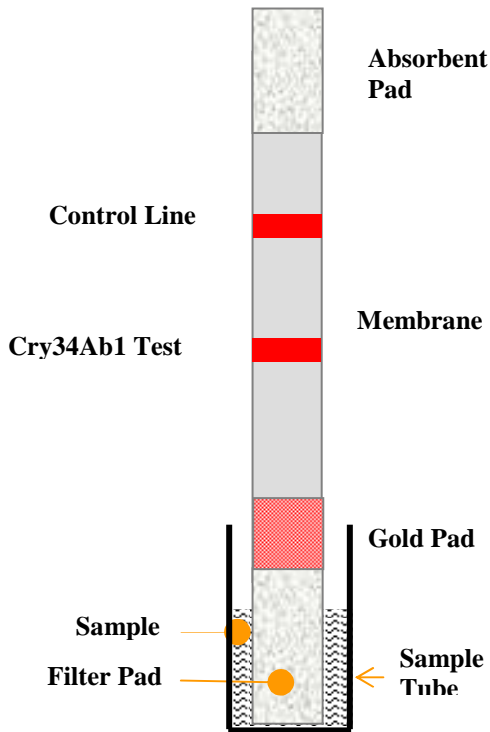

Interpreting the Lateral Flow Strip Test

Check the result window at five (5) minutes after inserting the strip. At least one line, the Control Line, should always develop approximately one (1) cm down from the Reservoir Pad. A red line in this position indicates that the device is functioning properly. A red line appearing below the Control Line is the Test Line and indicates a positive result. If the test strip displays two (2) red lines, the test is complete and the sample is positive for Cry34Ab1 corn. If at 5 minutes the test strip only shows a clearly visible Control Line, then the sample is negative for Cry34Ab1 corn. If no control line develops, the result is inconclusive and need to be repeated.

Note: *Test strip results should be interpreted after 5 minutes. Test strips interpreted after 10 minutes are invalid.*


Illustration of Positive and Negative Results



Example of an unreacted, negative (1-line) and positive (2-lines) test strip

Archiving Test Strips

If it is desired to archive test strip results, cut off the bottom and top strip pads as illustrated below within one (1) hour of test completion.

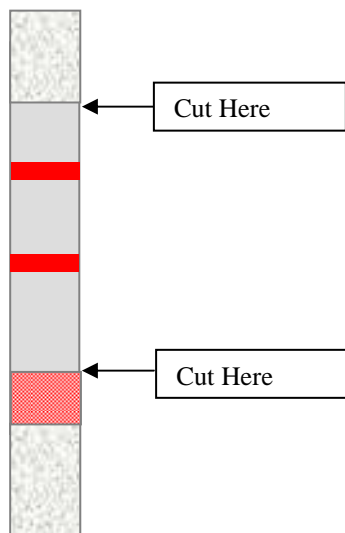

Equipment Cleaning and Drying

Caution: It is important to clean and dry the jars and cutting blades between samples.

1. The “Mason” jar should be emptied, rinsed thoroughly with water and completely dried with a paper towel between uses.
2. The cutting blades for the blender should be rinsed with water until **all ground corn** is removed, washed using standard household liquid soap, rinsed well and carefully dried. If available, spraying or rinsing with methanol or isopropyl (rubbing) alcohol will assist drying.

Principle of the Screening Application

Screening at Very Low GM Levels

Screening grain at very low GM levels can be accomplished by using a sufficiently large sample size that tests negative for the GM trait. Lateral flow strips can be used by testing multiple sub-samples the size, of which, do not exceed the sensitivity of the strip test. **The Trait✓ Cry34Ab1 strip test sensitivity is at least one HERCULEX RW or HERCULEX XTRA kernel in 800.**

The Trait✓ Cry34Ab1 Test Strip provides a yes/no answer for the presence or absence of Cry34Ab1 corn in a given sample. Testing multiple statistically selected sub-samples allows an estimate of the percent of Cry34Ab1 corn. The test results provide information about the probability of the percent Cry34Ab1 corn in the sample.

Note: The test protocol does not determine the exact percent of Cry34Ab1 corn kernels. It determines the probability that a sample contains greater or less than a specified threshold concentration.

P/N 3090056

Statistical Interpretation

The following tables provide information at five confidence levels with the use of multiple samples of 400 kernels 600 kernels or 800 kernels each. The tables provide the maximum percent GM levels that would be expected in the sample if all test-samples provide negative results. Either table can be used depending on the desired screening level and how the samples will be processed.

**Table C: 400 Seed Sub-Samples
(All Sub-Samples Must be Negative)**

No. Sub-Samples of 400 Seeds Each	Percent GM using Sub-Sample Sizes of 400 Seeds at Five Different Confidence Levels (%)				
	50	75	90	95	99
1	0.17	0.35	0.58	0.75	1.2
2	0.087	0.18	0.29	0.38	0.58
3	0.058	0.12	0.20	0.25	0.39
4	0.045	0.085	0.15	0.19	0.29
5	0.035	0.070	0.12	0.15	0.25
6	0.029	0.058	0.10	0.13	0.20
7	0.025	0.050	0.085	0.11	0.18
8	0.022	0.044	0.075	0.10	0.15

**Table D: 600 Seed Sub-Samples
(All Sub-Samples Must be Negative)**

No. Sub-Samples of 600 Seeds Each	Percent GM using Sub-Sample Sizes of 600 Seeds at Five Different Confidence Levels (%)				
	50	75	90	95	99
1	0.12	0.23	0.39	0.50	0.78
2	0.058	0.12	0.20	0.25	0.39
3	0.039	0.077	0.13	0.17	0.27
4	0.029	0.058	0.10	0.13	0.20
5	0.024	0.047	0.077	0.10	0.16
6	0.019	0.039	0.065	0.085	0.13
7	0.017	0.033	0.055	0.075	0.11
8	0.015	0.029	0.050	0.065	0.096

**Table E: 800 Seed Sub-Samples
(All Sub-Samples Must be Negative)**

No. Sub-Samples of 800 Seeds Each	Percent GM using Sub-Sample Sizes of 800 Seeds at Five Different Confidence Levels (%)				
	50	75	90	95	99
1	0.087	0.175	0.288	0.375	0.575
2	0.044	0.087	0.144	0.187	0.285
3	0.029	0.058	0.096	0.125	0.192
4	0.022	0.044	0.072	0.094	0.145
5	0.017	0.035	0.058	0.075	0.115
6	0.015	0.029	0.048	0.063	0.097
7	0.013	0.025	0.041	0.054	0.083
8	0.011	0.022	0.036	0.047	0.072

Warranties and Liabilities

Strategic Diagnostics Inc. (“SDI”) warrants the Products manufactured by it will be free of defects in materials and workmanship when used in accordance with the applicable instructions for a period equal to the shorter of one year from date of shipment of the Product(s) or the expiration date marked on the Product packaging. Application protocols published by SDI are intended to be only guidelines for the Buyers of the Products. Each Buyer is expected to validate the applicability of each application protocol to in their individual applications. **SDI MAKES NO OTHER WARRANTY, EXPRESSED OR IMPLIED. THERE IS NO WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE.**

SDI’s sole obligation with respect to the foregoing warranties shall be, at its option, to either replace or to refund the purchase price of the Product(s) or part thereof that proves defective in materials or workmanship within the warranty period, provided the customer notifies SDI promptly of any such defect. **SDI SHALL NOT BE LIABLE FOR ANY DIRECT, INDIRECT OR CONSEQUENTIAL DAMAGES RESULTING FROM ECONOMIC LOSS OR PROPERTY DAMAGES SUSTAINED BY BUYER OR ANY CUSTOMER FROM THE USE OF THE PRODUCT (S).**

For Technical Service call:

Strategic Diagnostics Inc
111 Pencader Drive
Newark, DE 19702

Phone: 800-544-8881
Fax: 302-456-6782
e-mail: techservice@sdix.com



HERCULEX™ is a trademark of Dow AgroSciences LLC.